


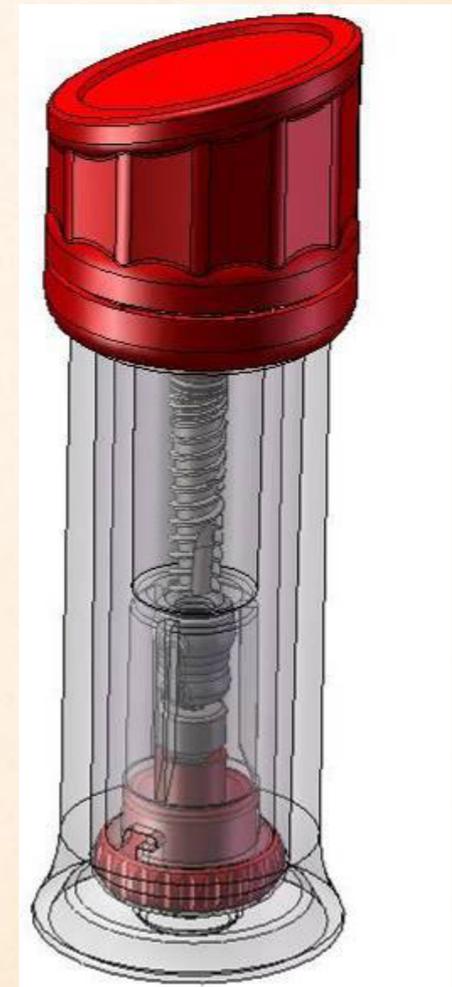
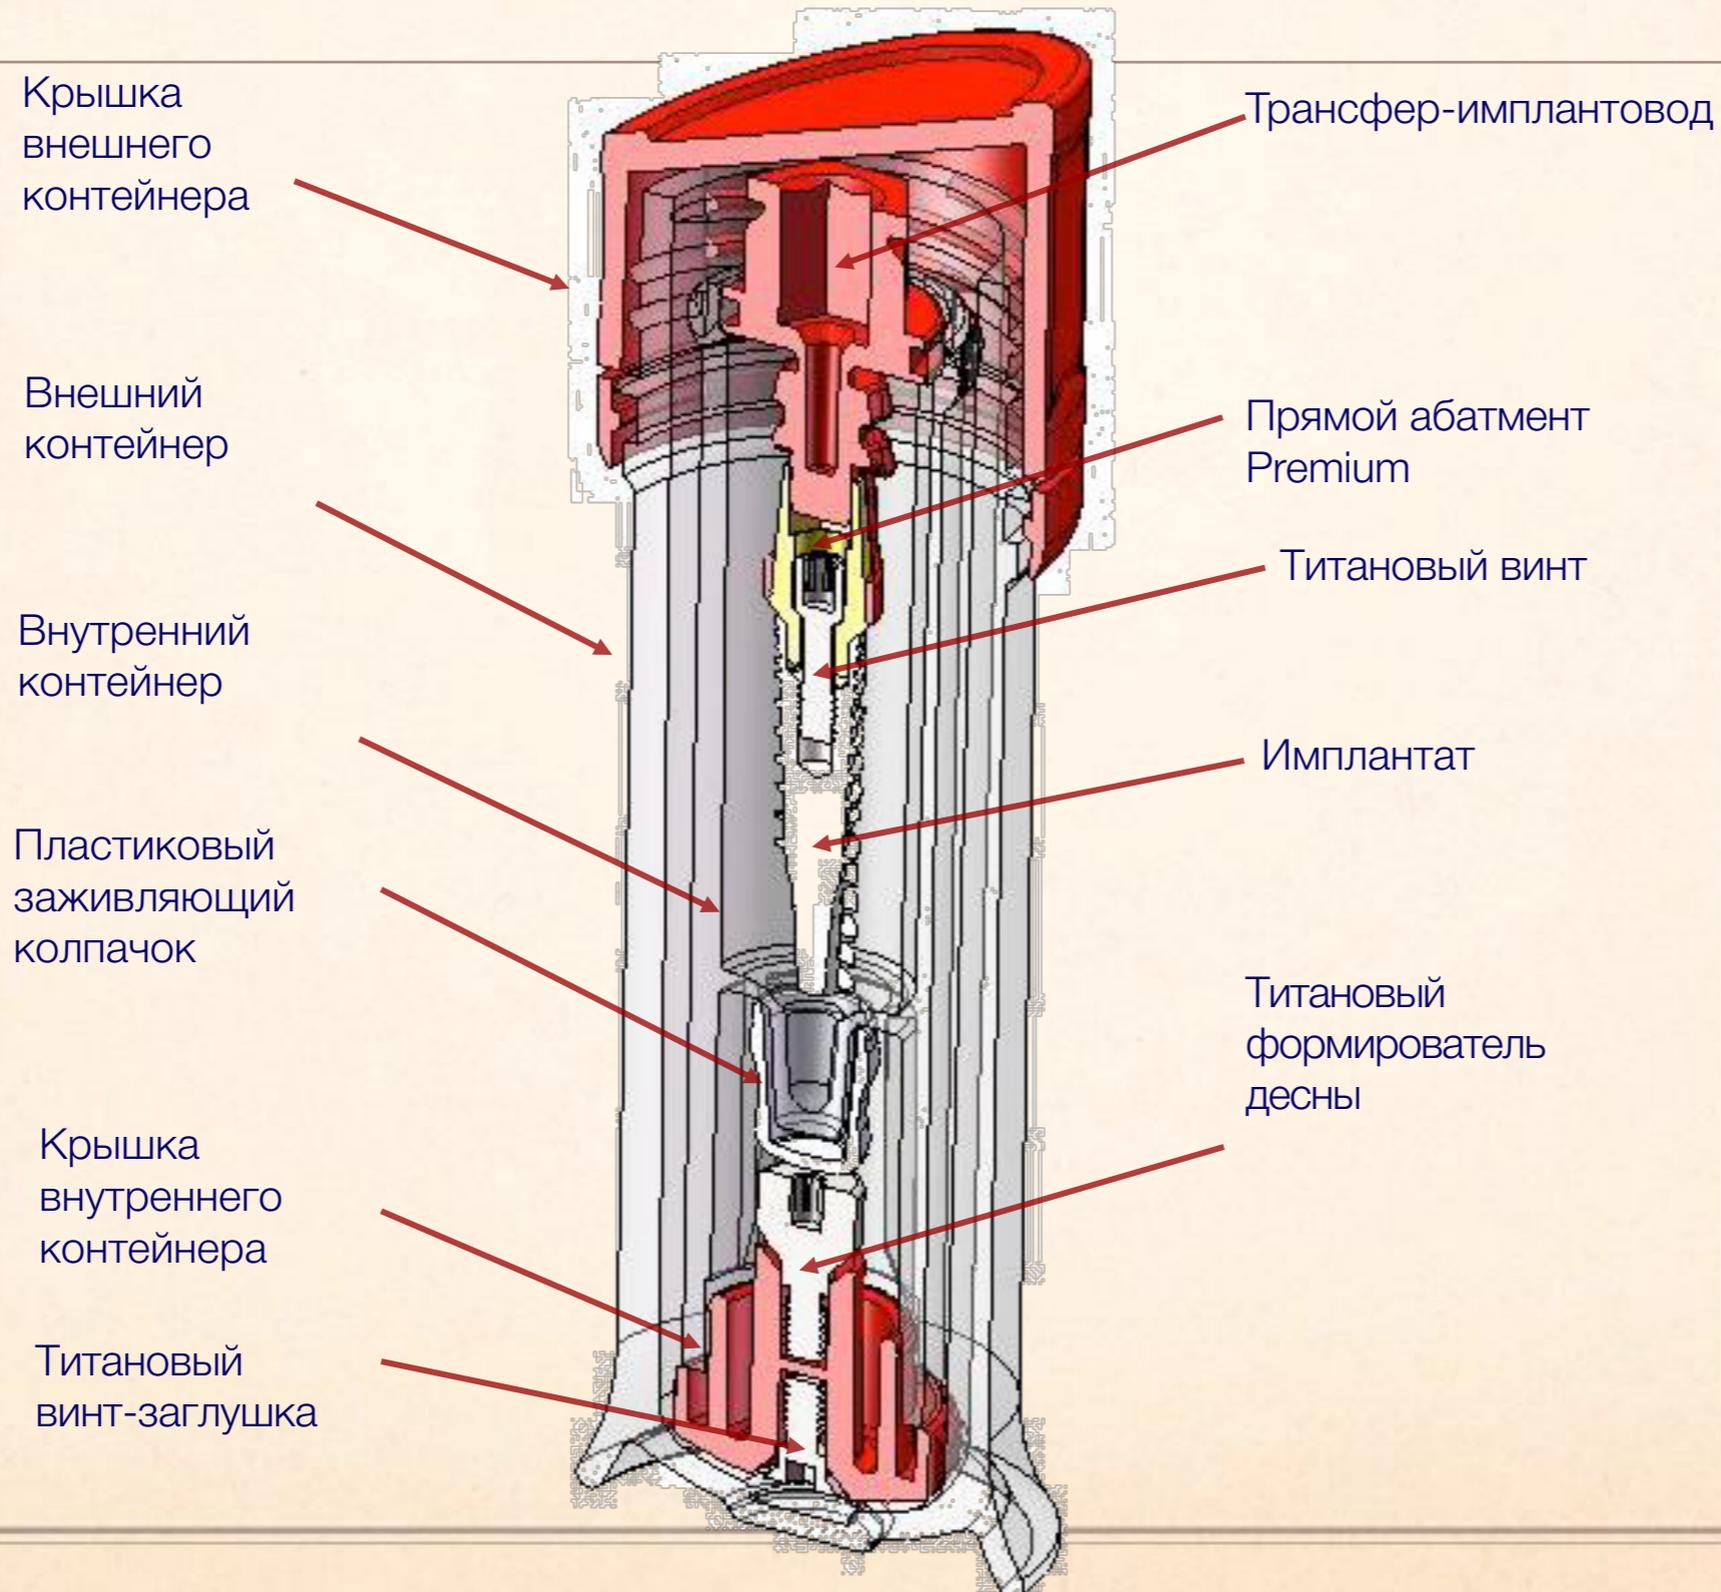
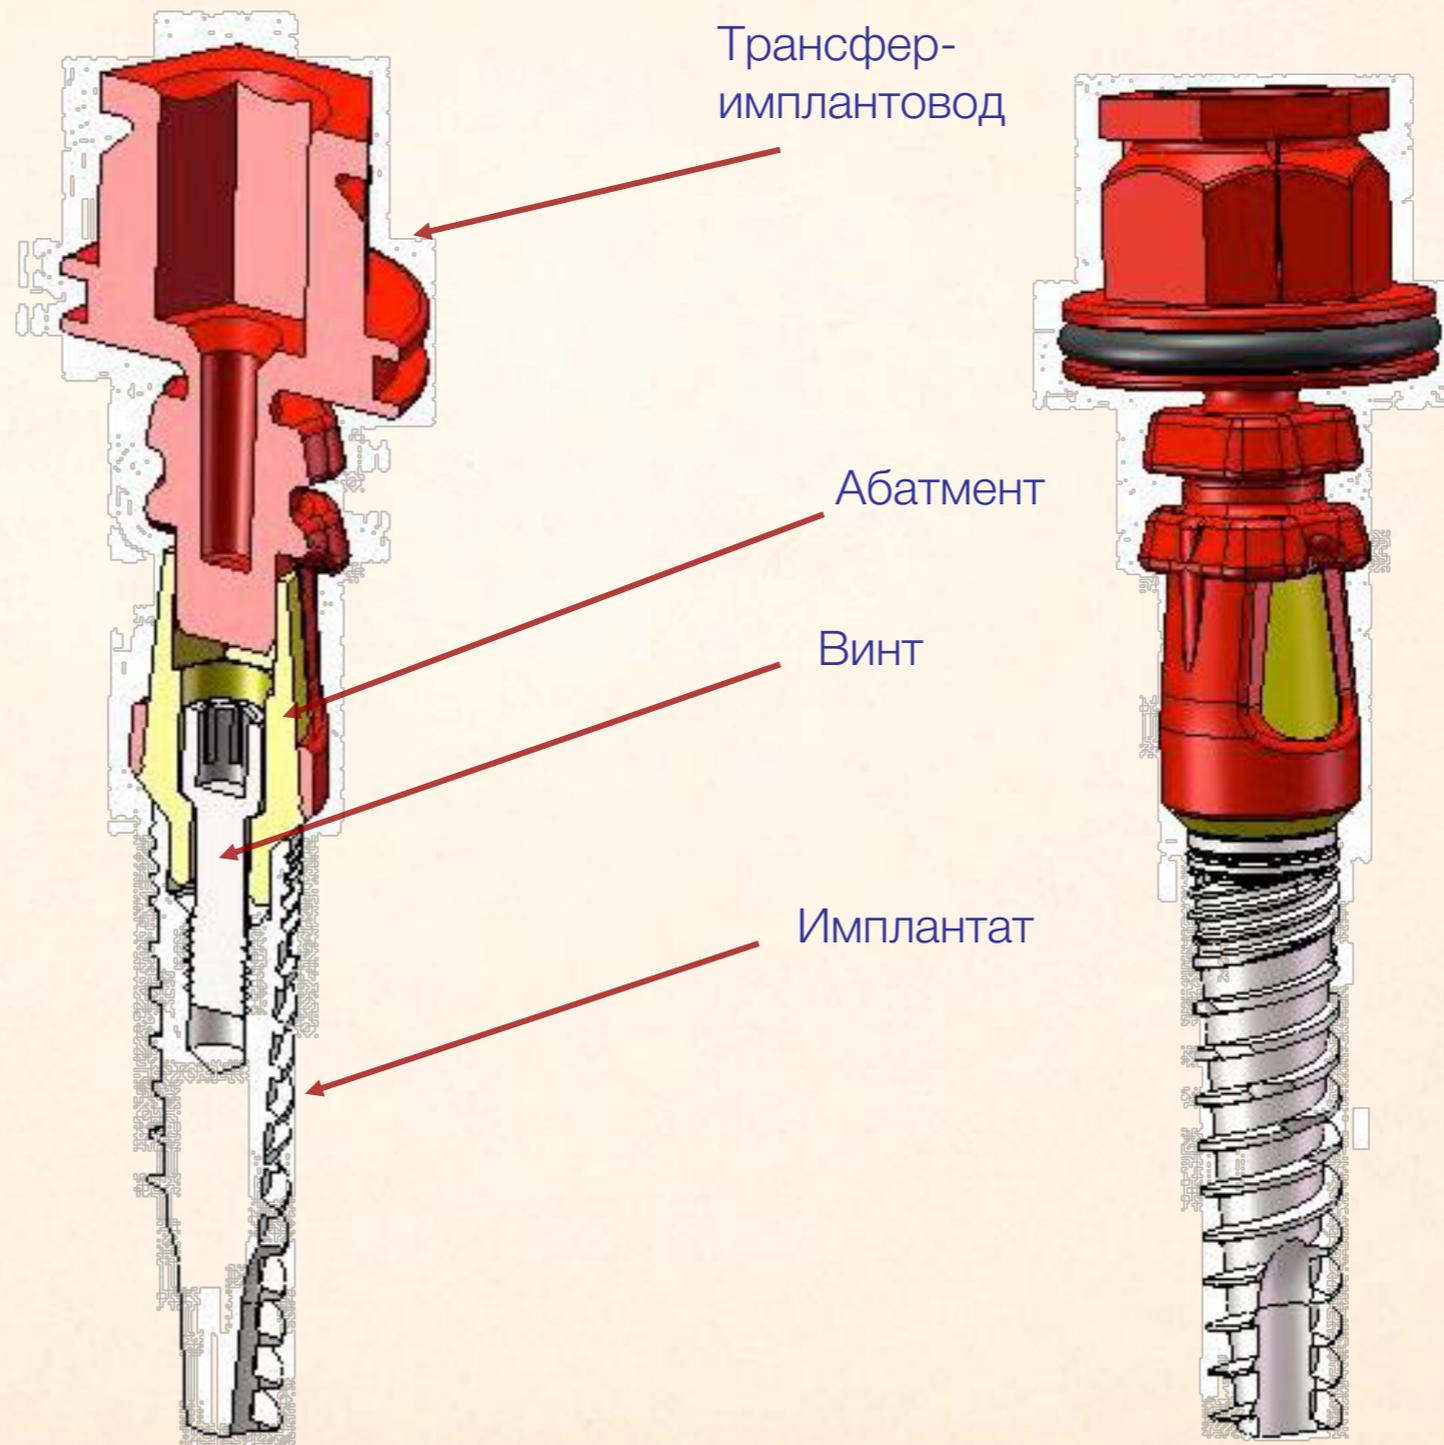



Комплектация Premium

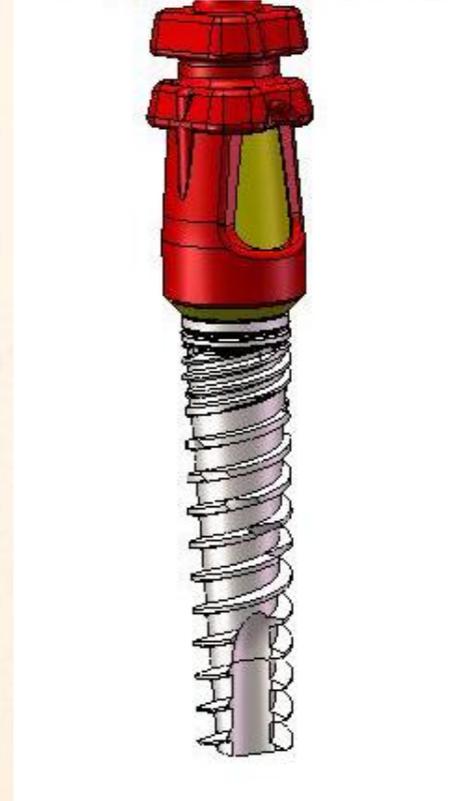

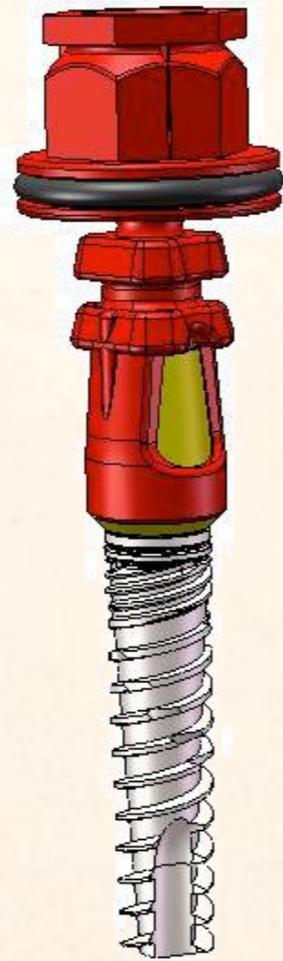

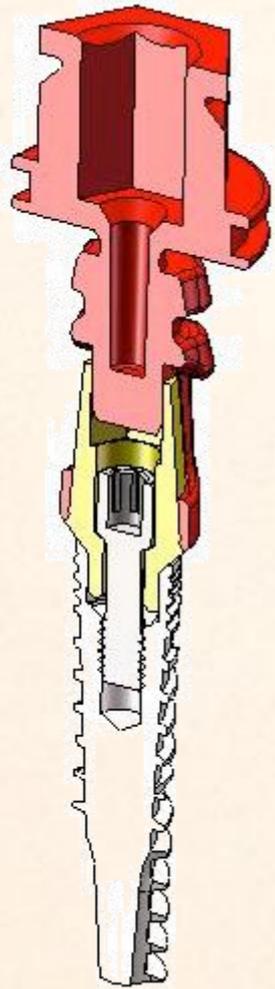

Трансфер может быть отделен от имплантовода и использован в лабораторных целях

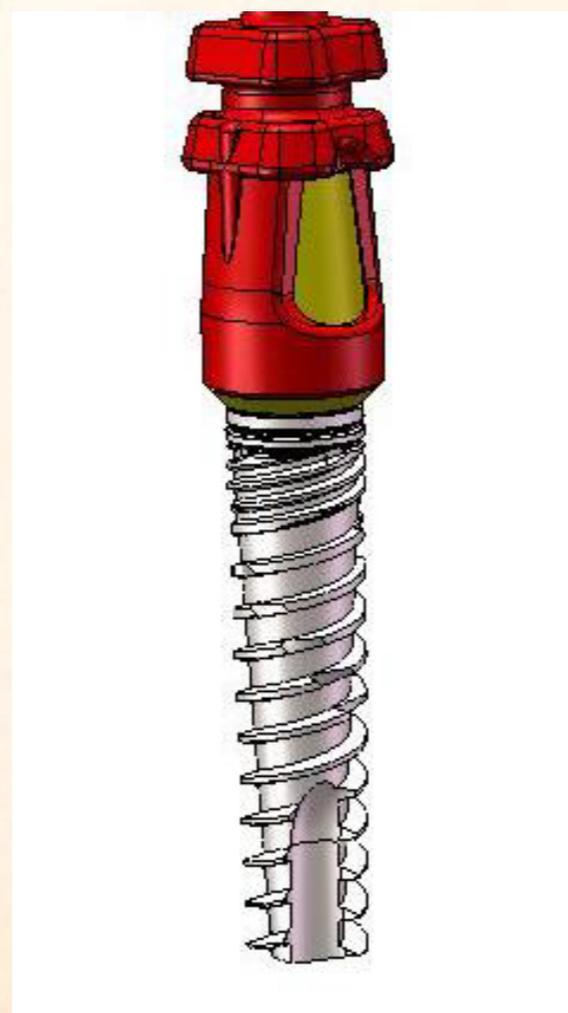











sterile packaged & pack
inspected or undamaged
2015-01

LOT 0912034

Ø3.111

CE

STERILE



ISO: 9001-2000
ISO: 13485:2003

ZIMIC



Sterility guaranteed if pack
Unopened or undamaged

2015-01

LOT 0912034D

Ø3:75
L11.5

CE

0473

ISO

DYNAMIC

Premium




CORTISONE

DYNAMIC L11.5 D3.75

LOT 0912034B

Premix II

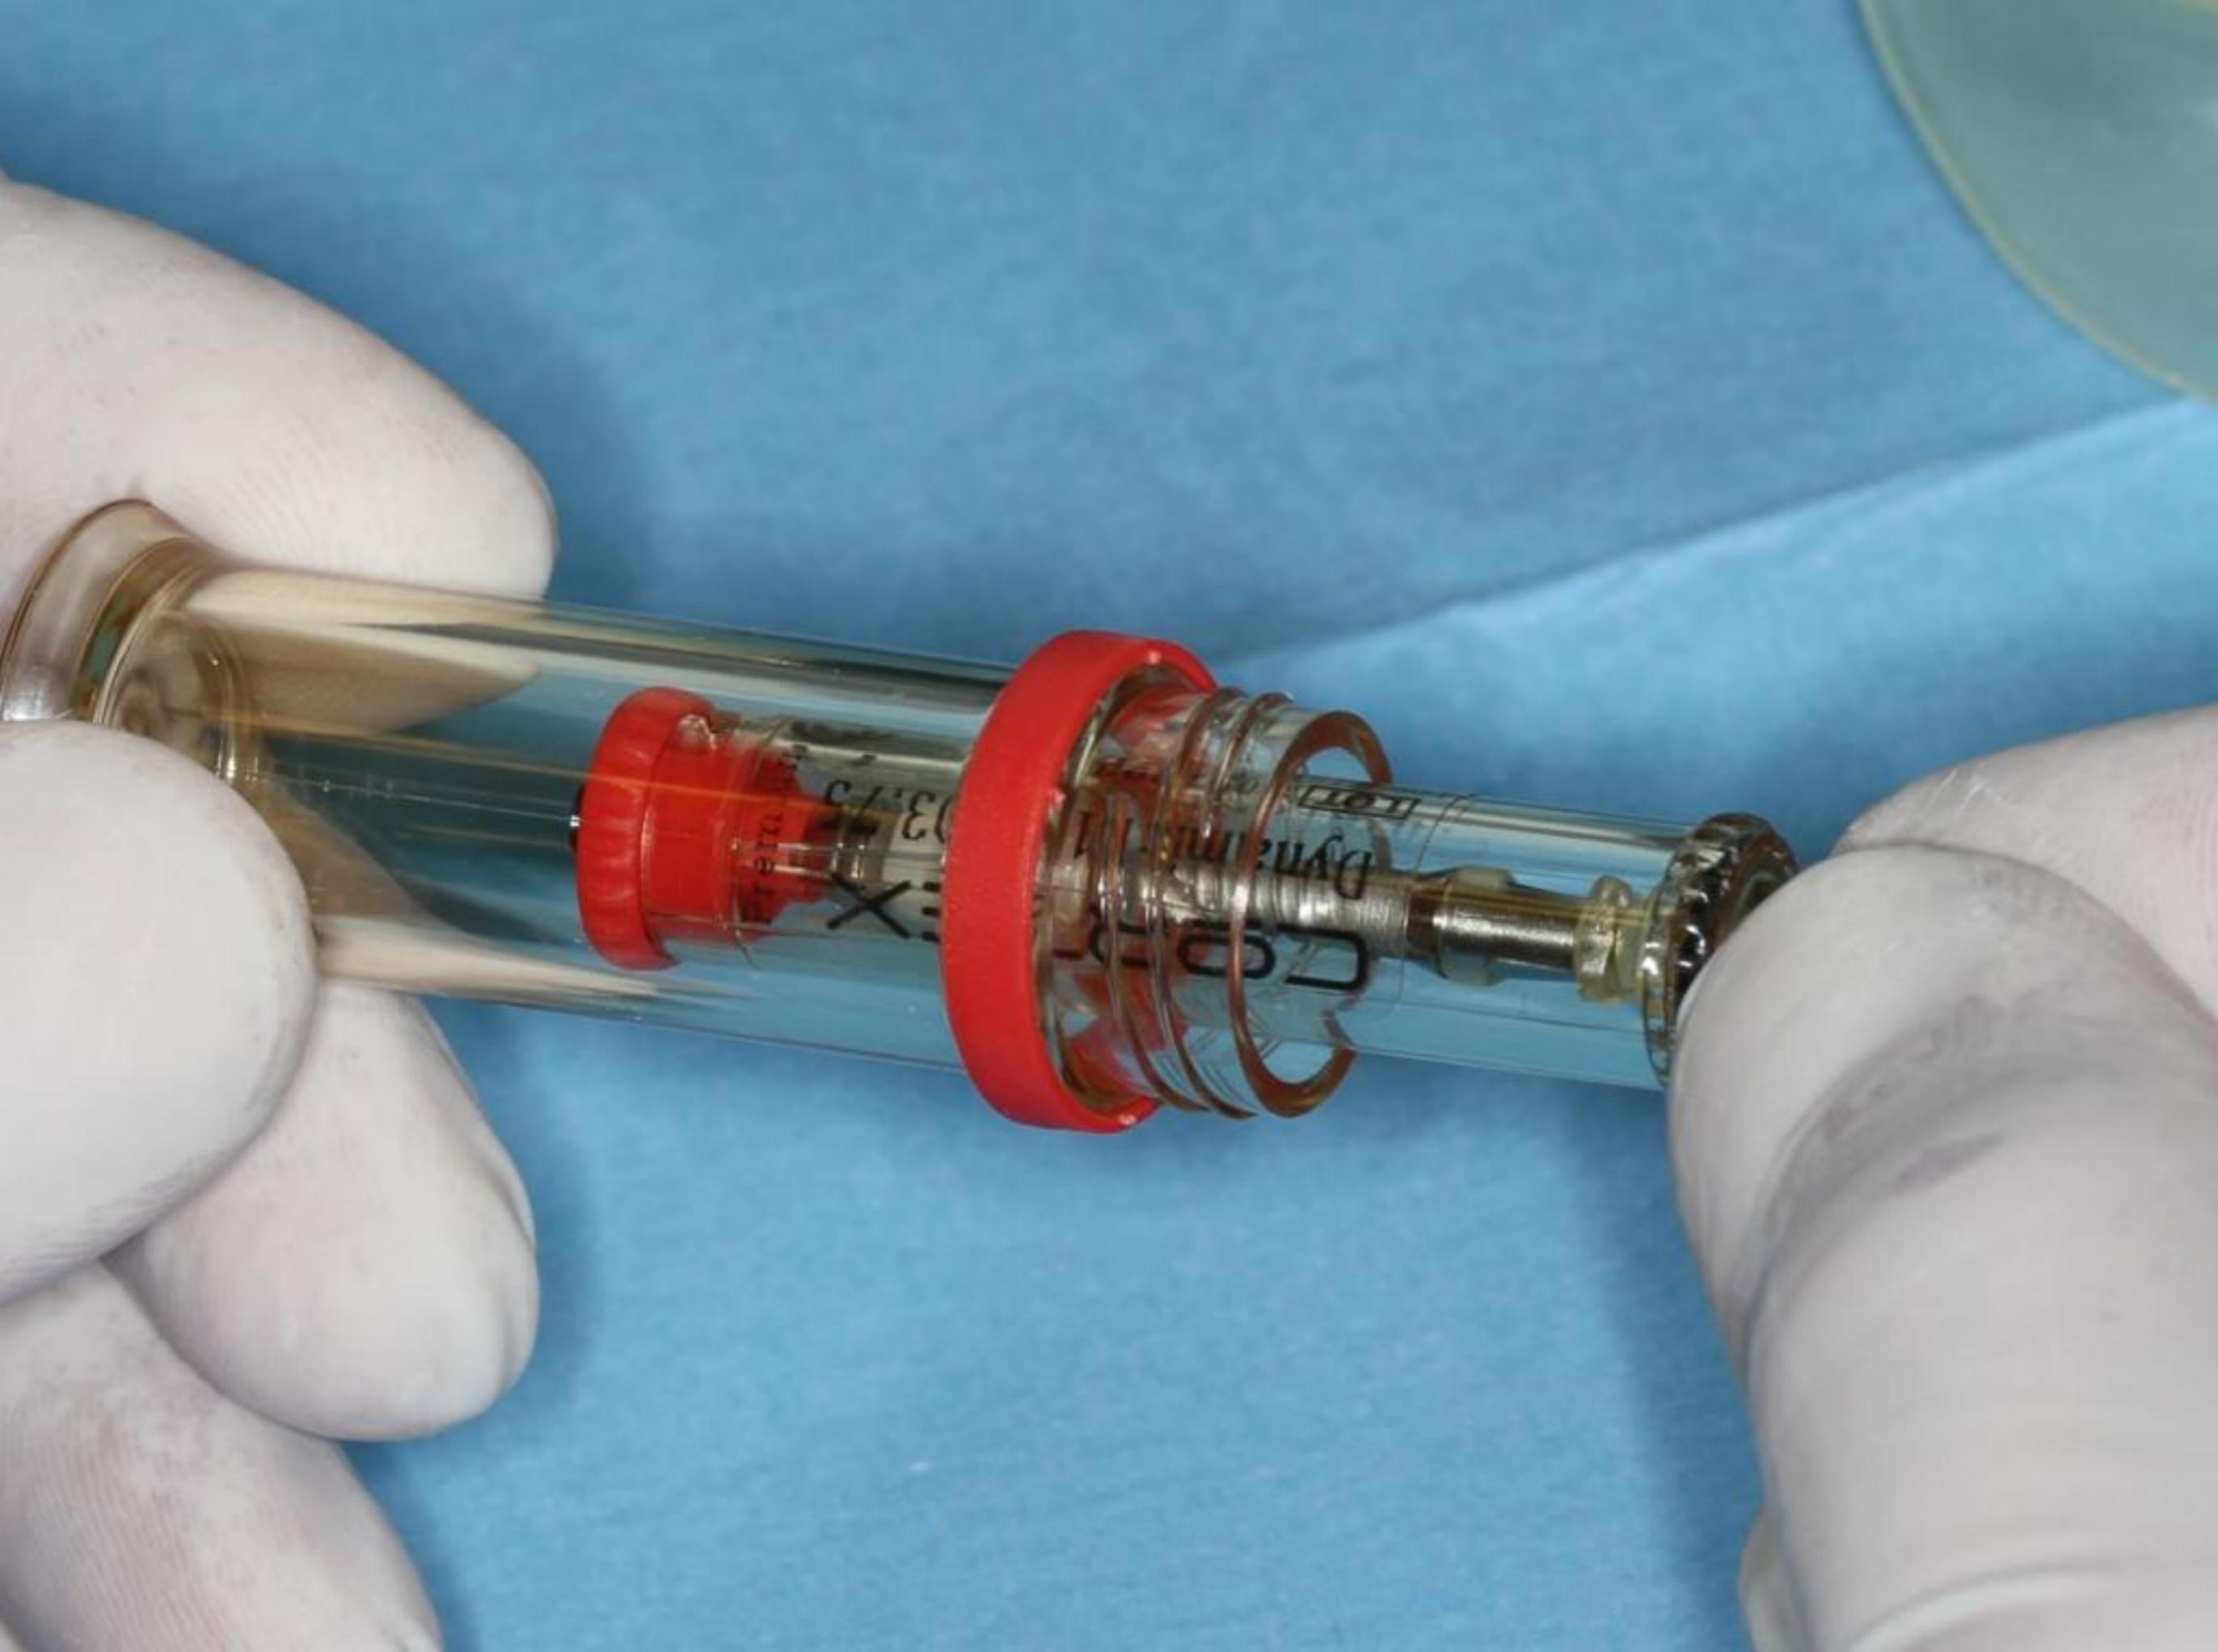










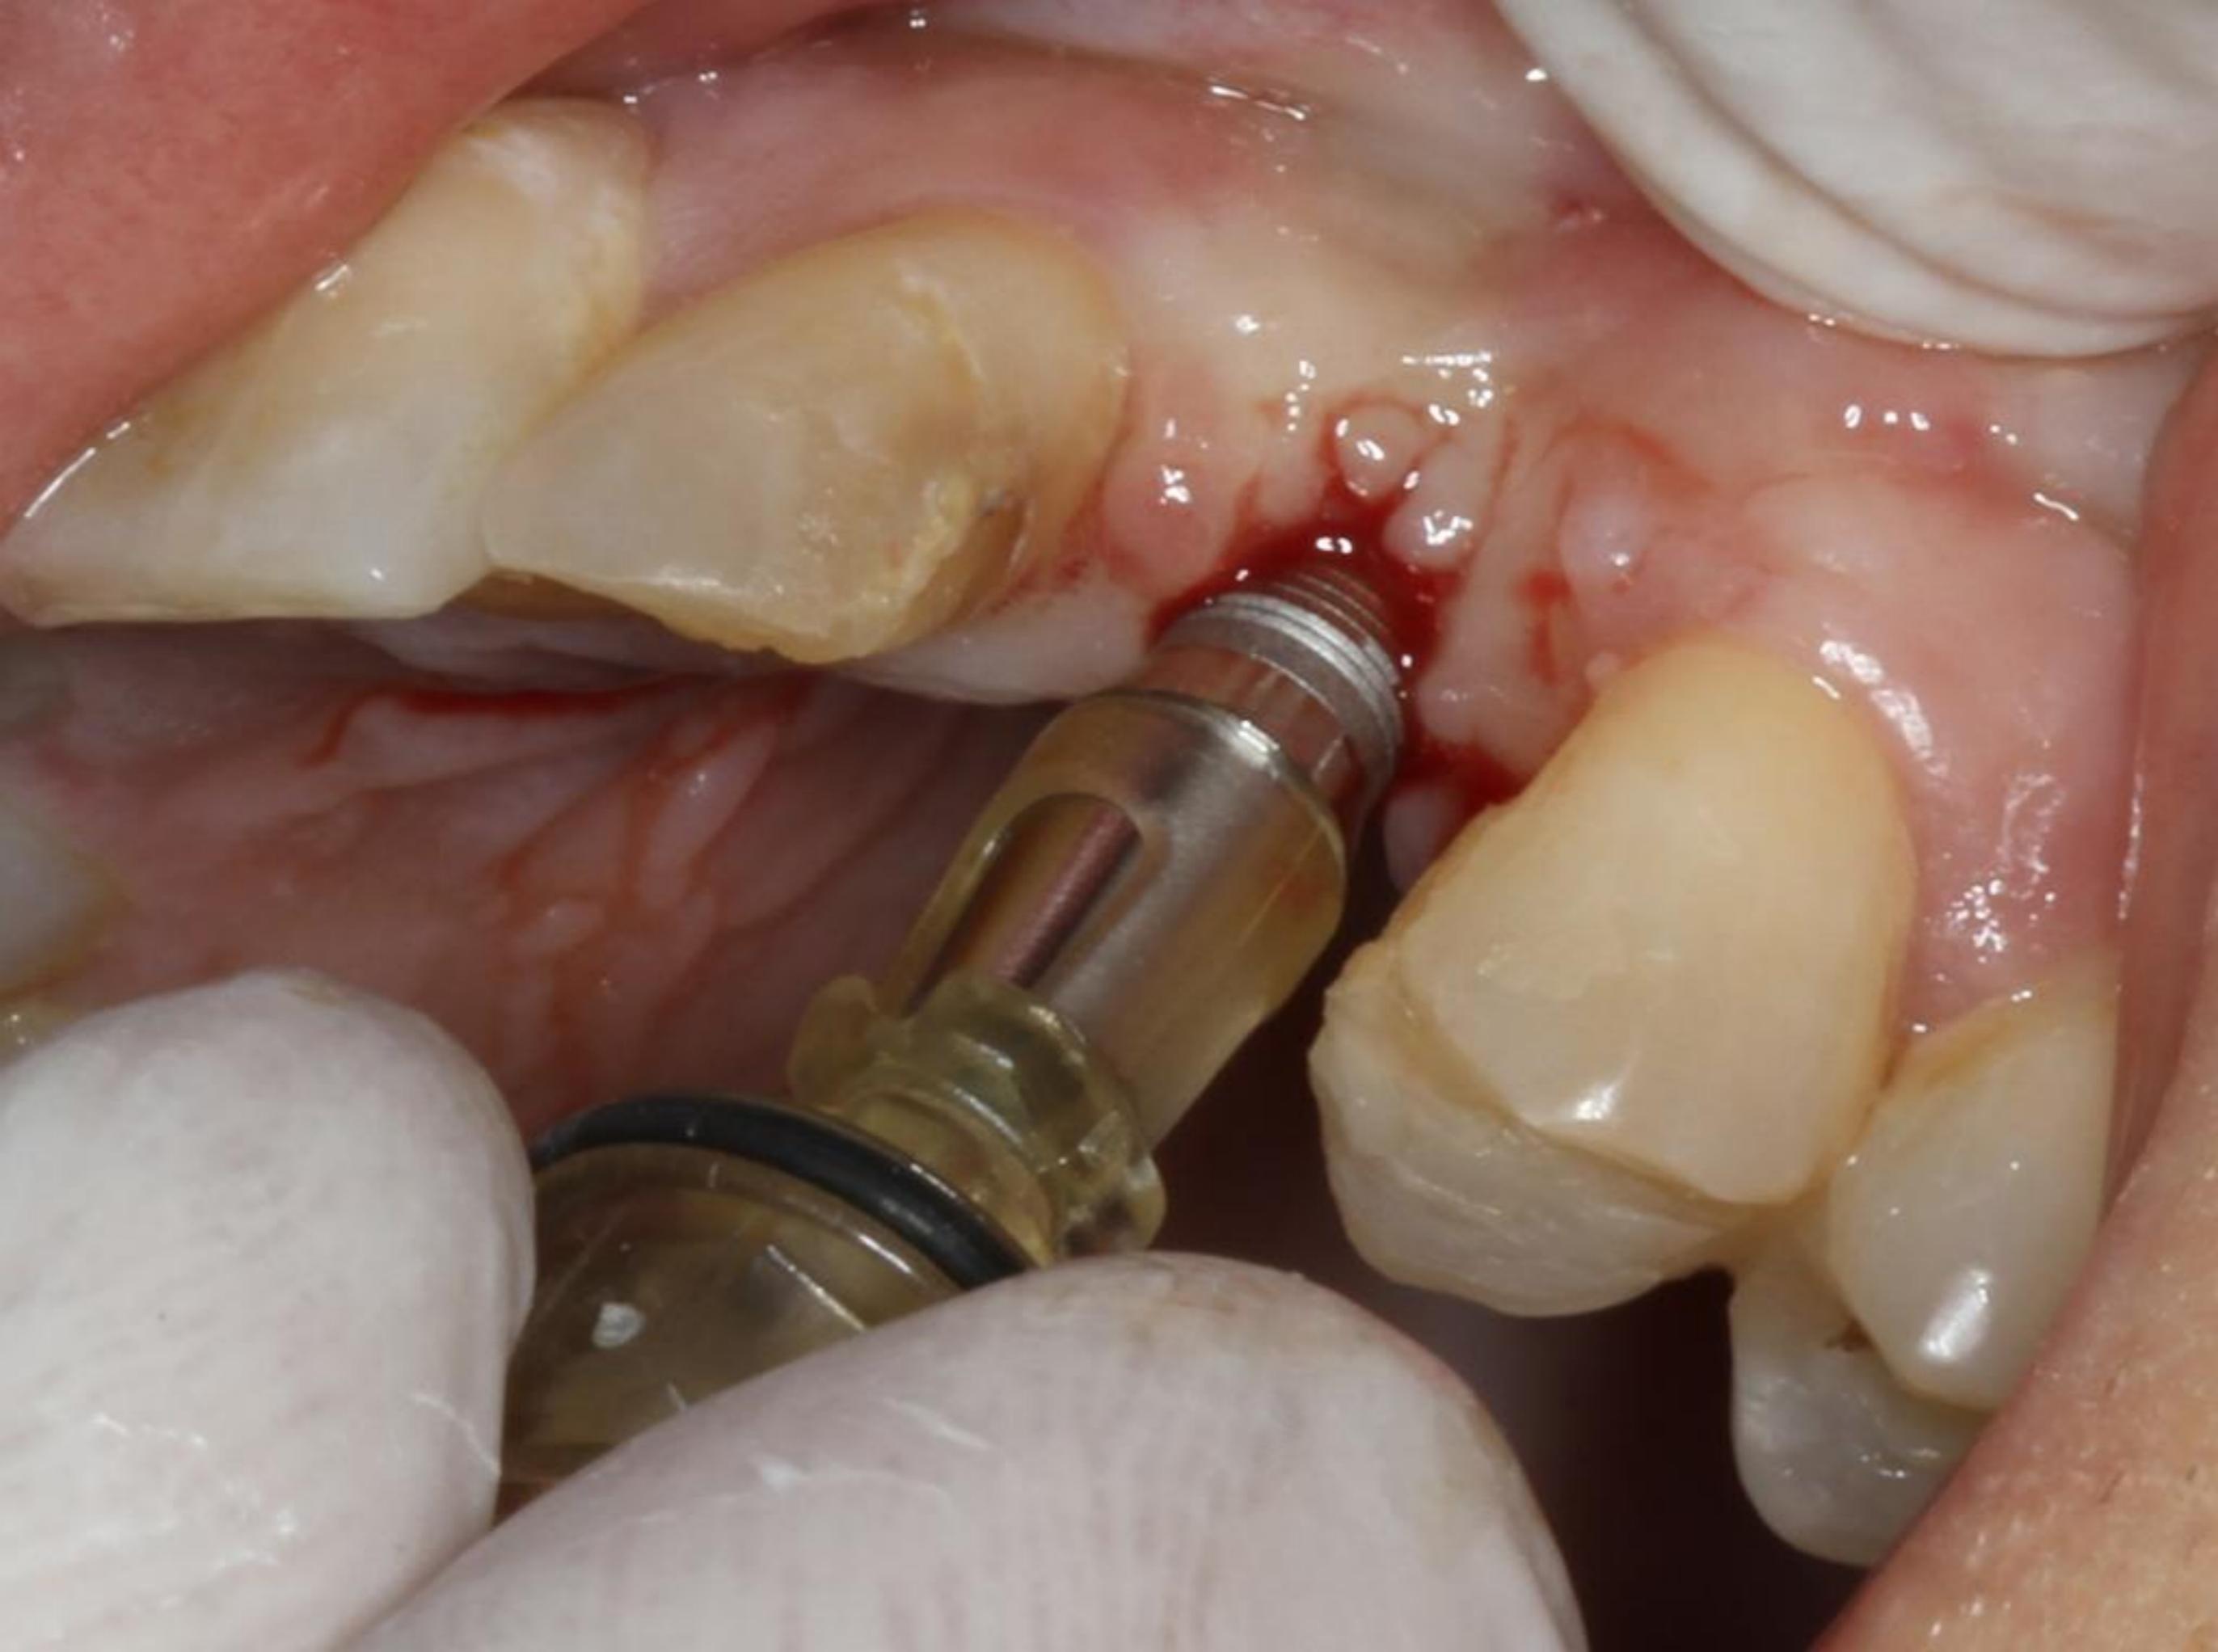











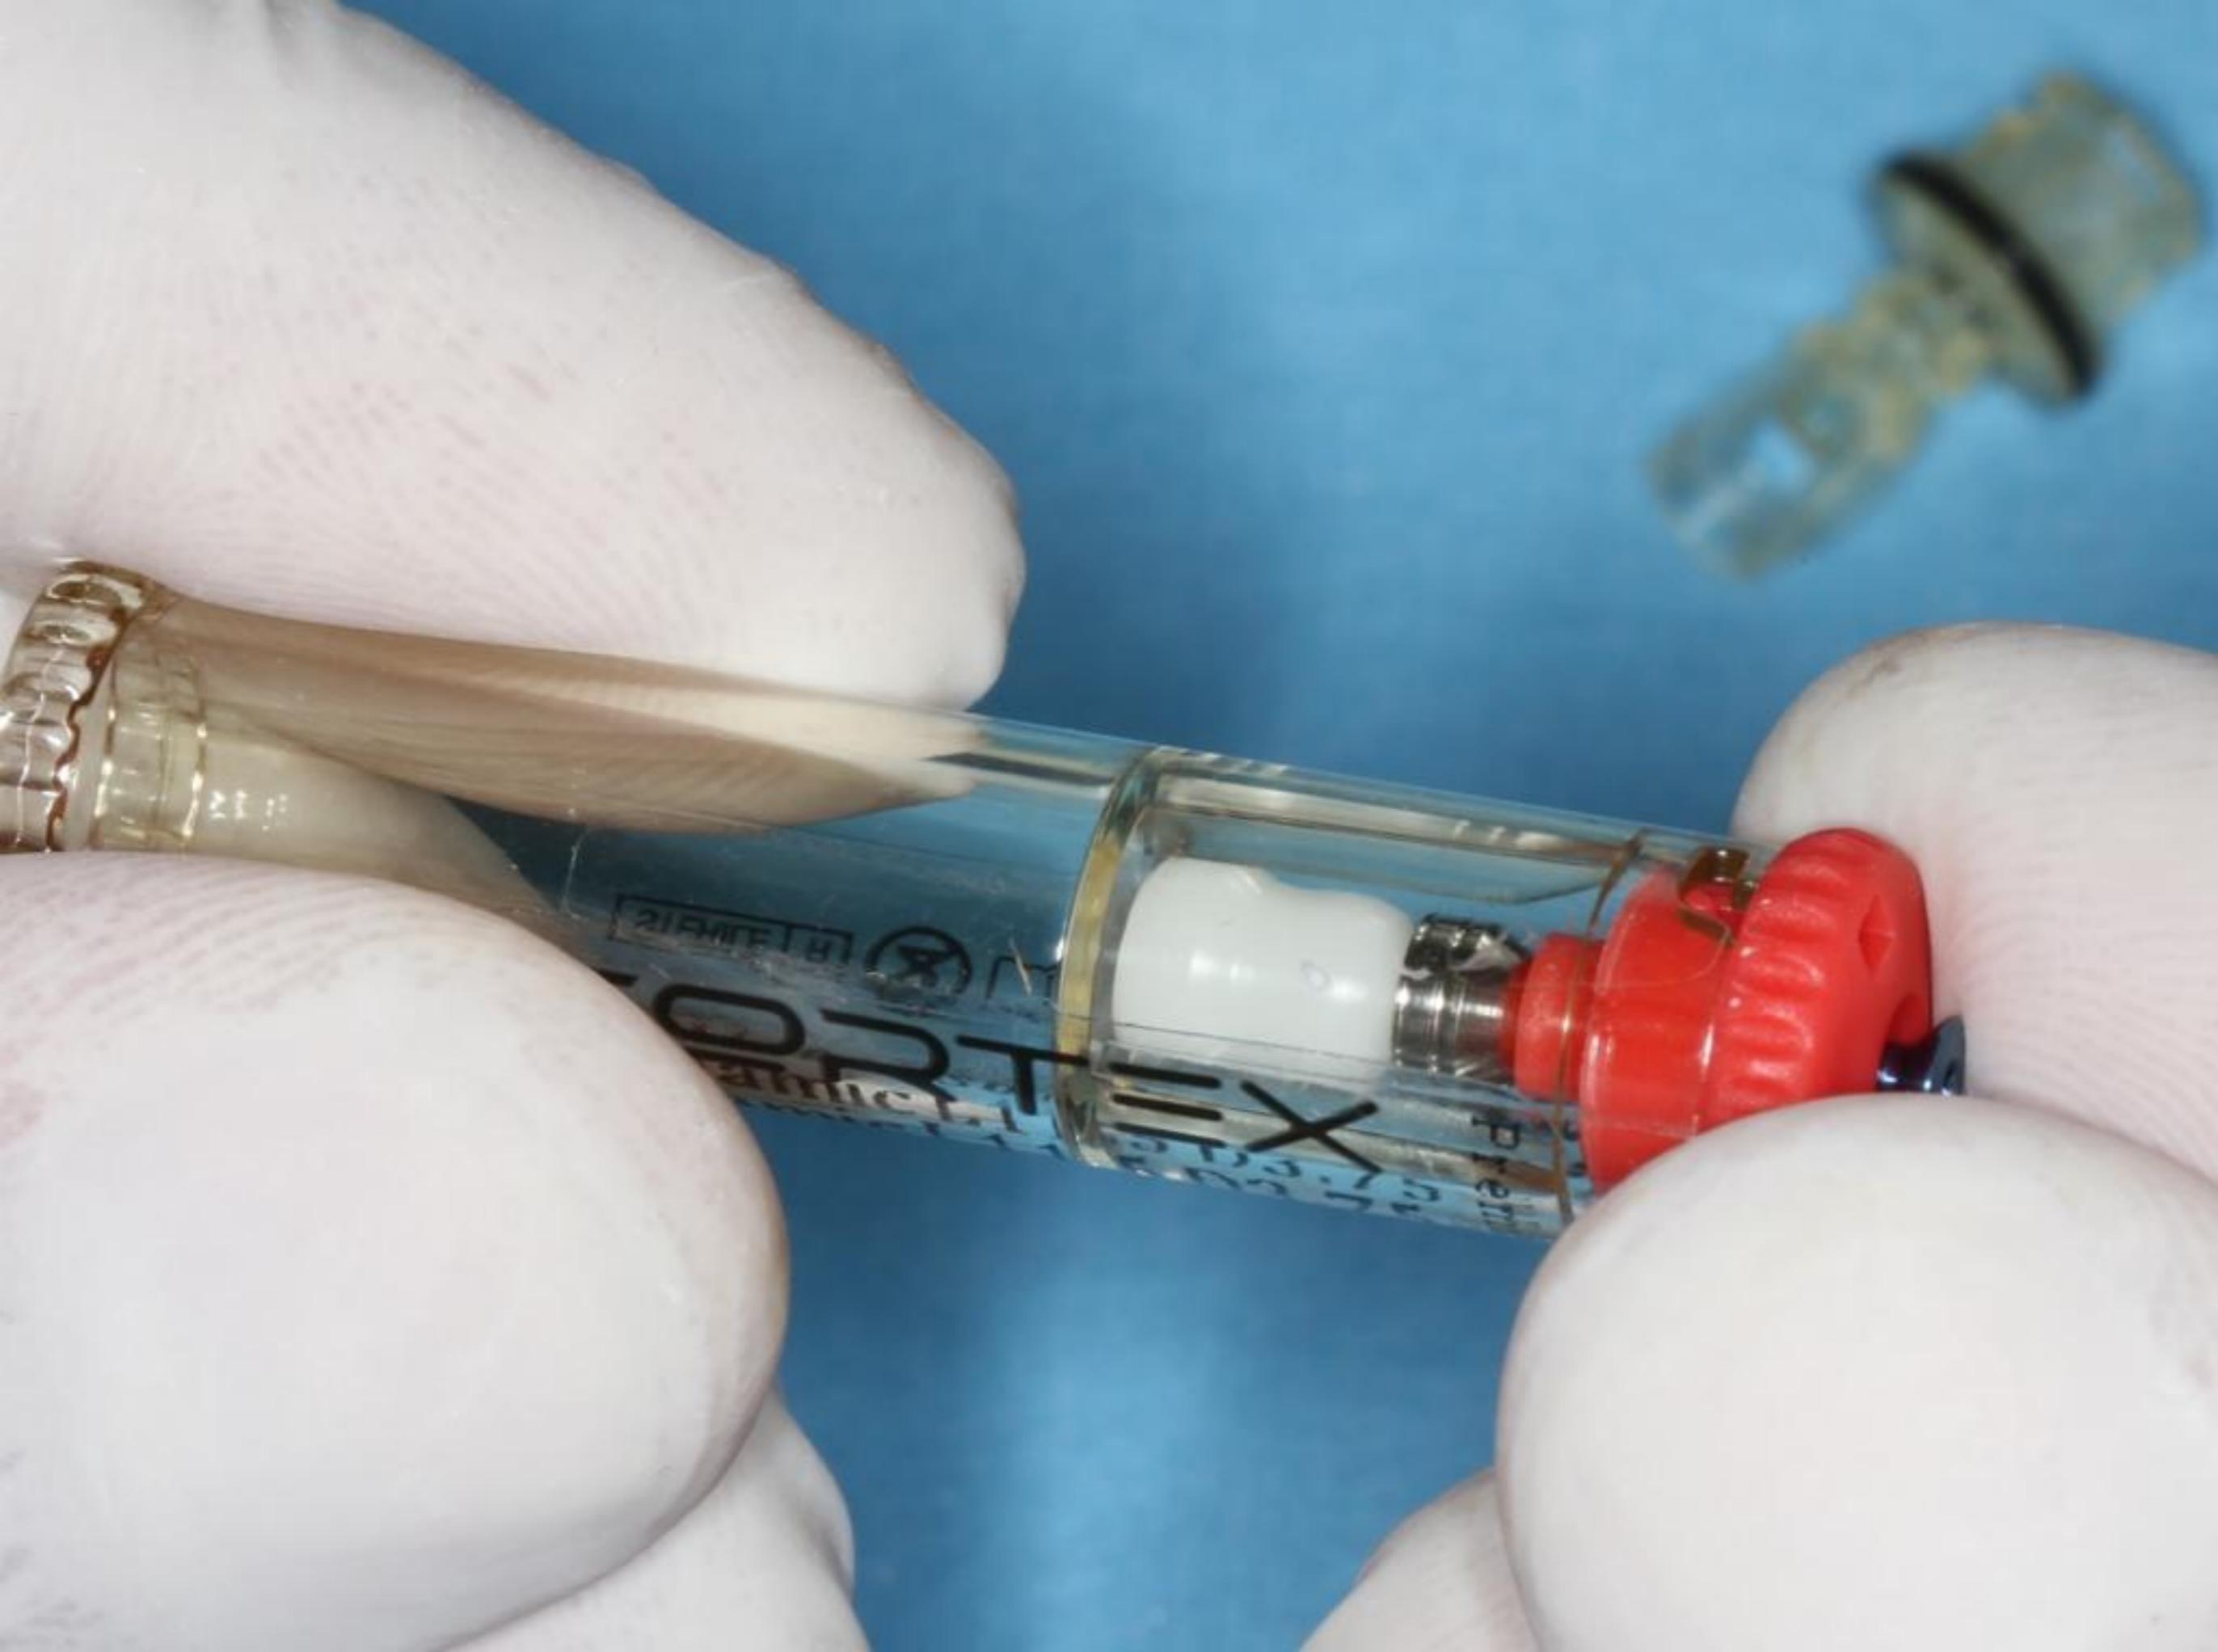

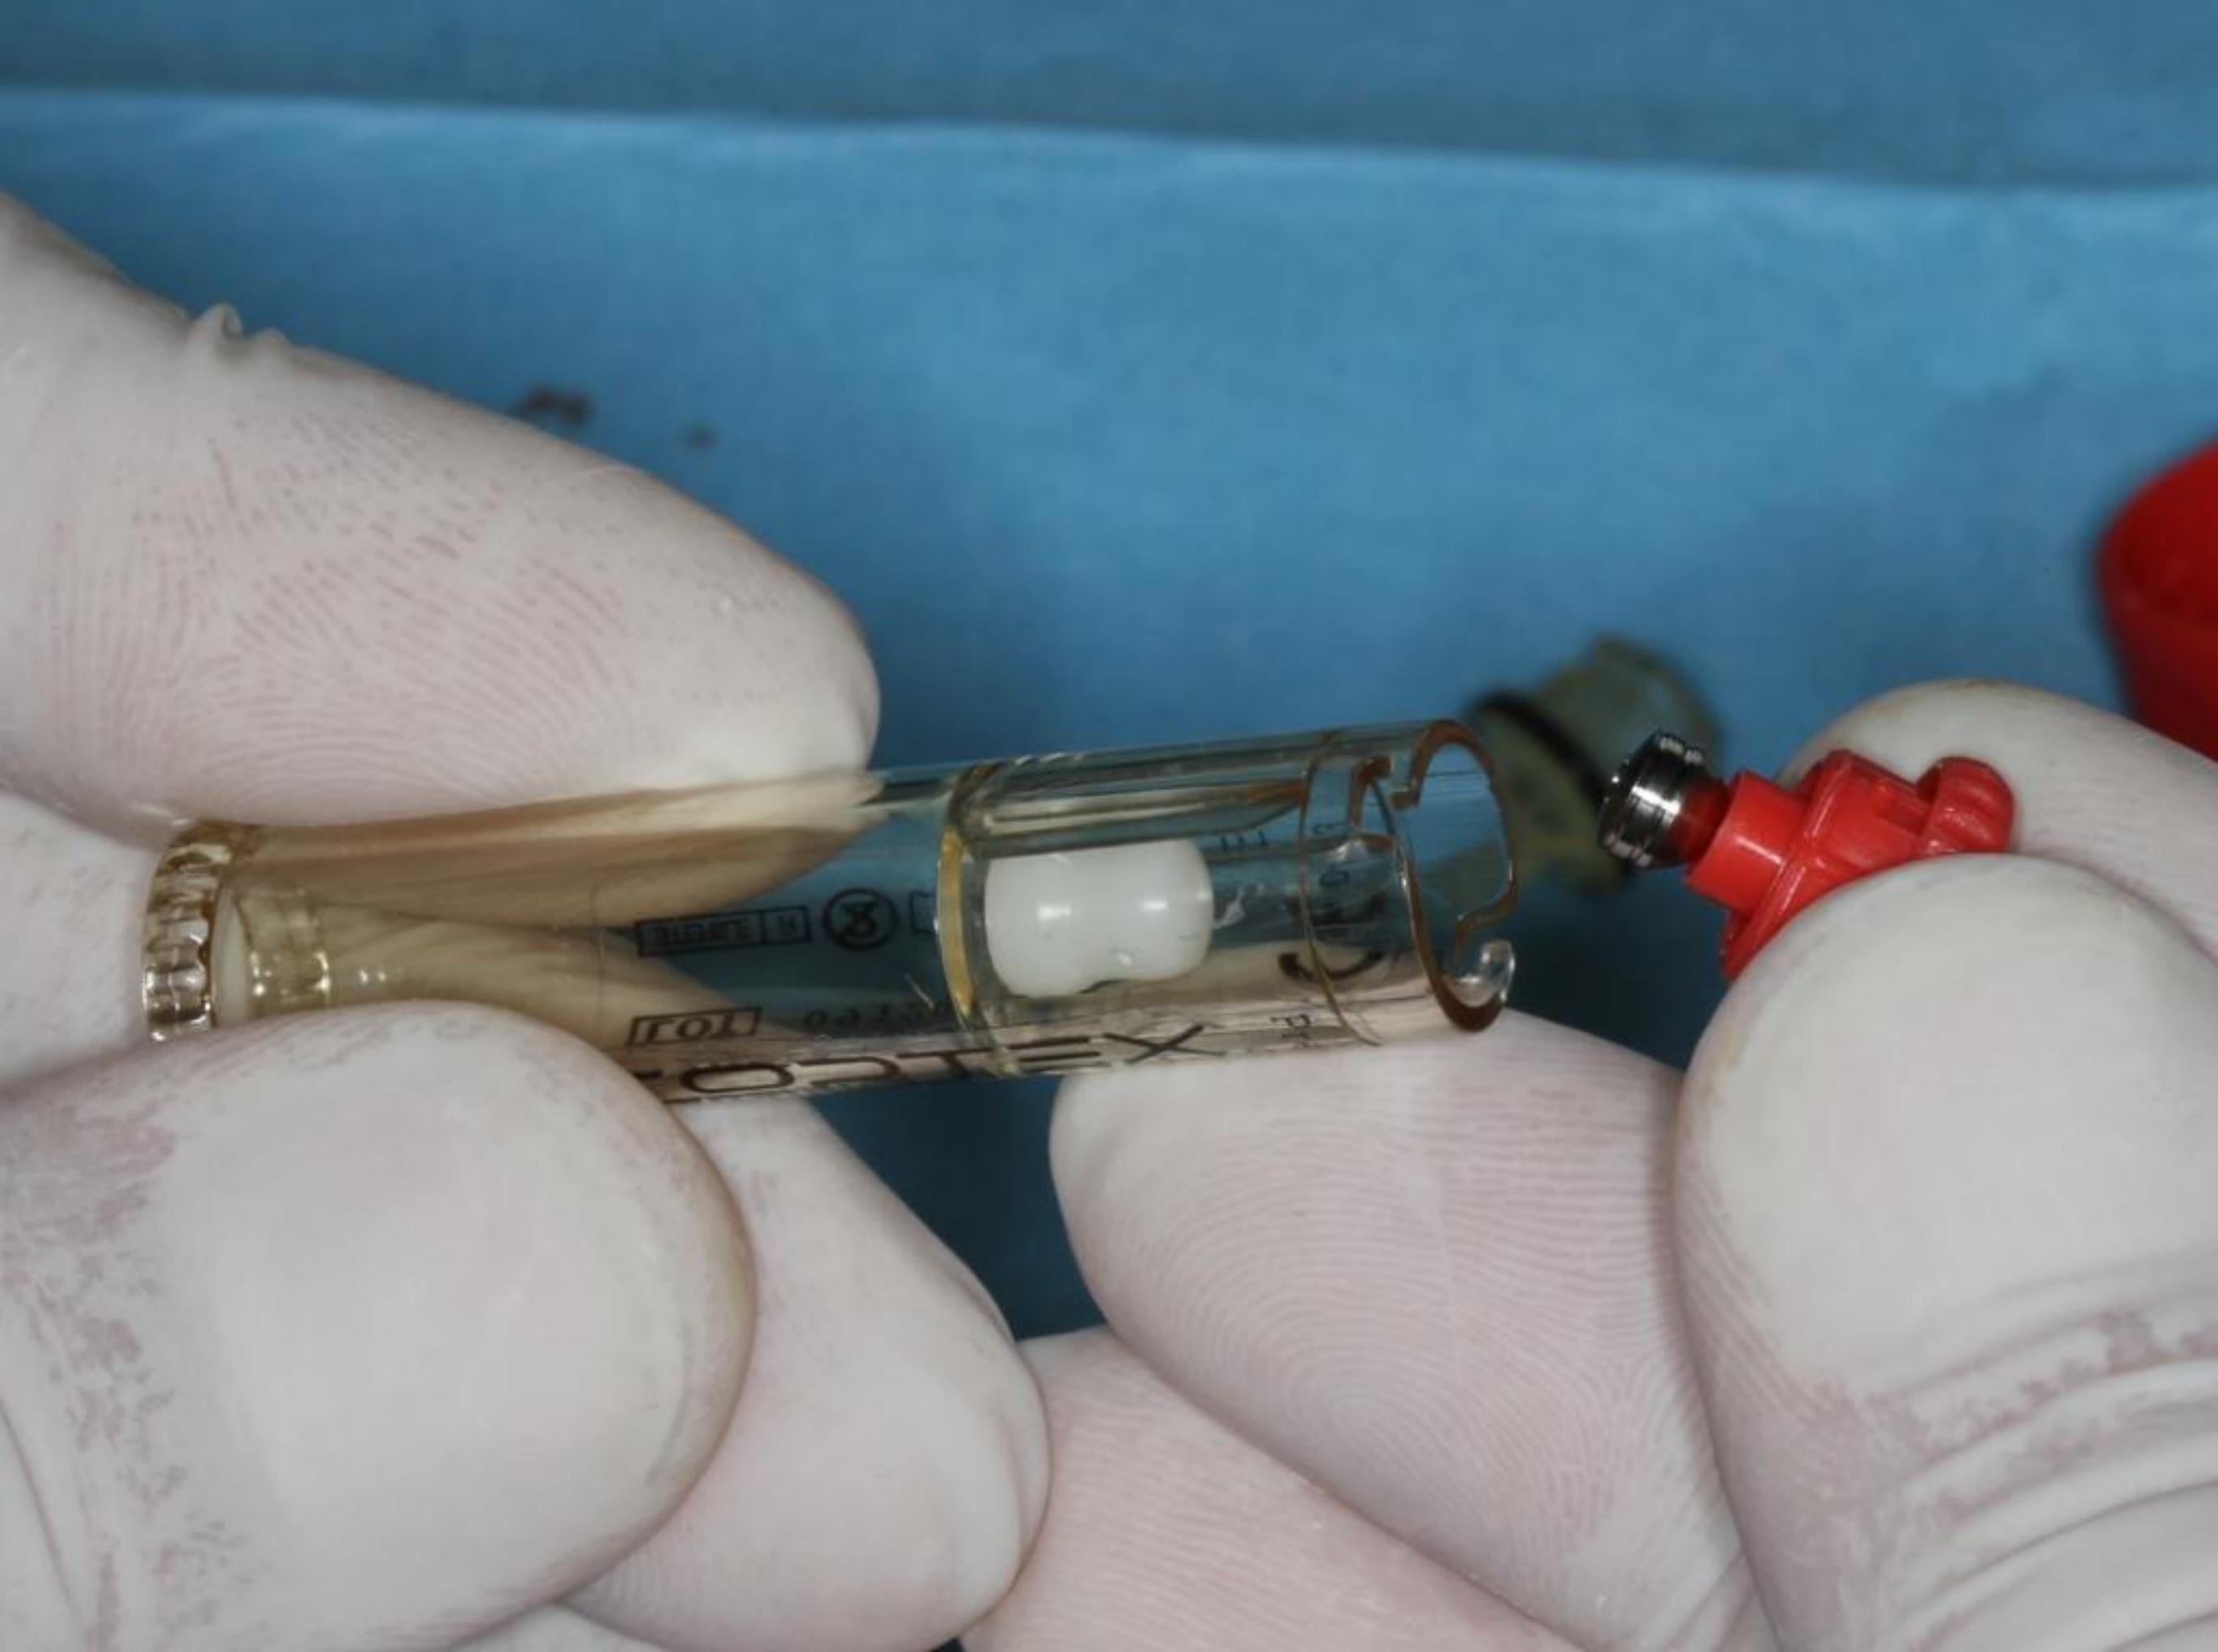



001503
DANSWICP
C05









